


FIG. 1

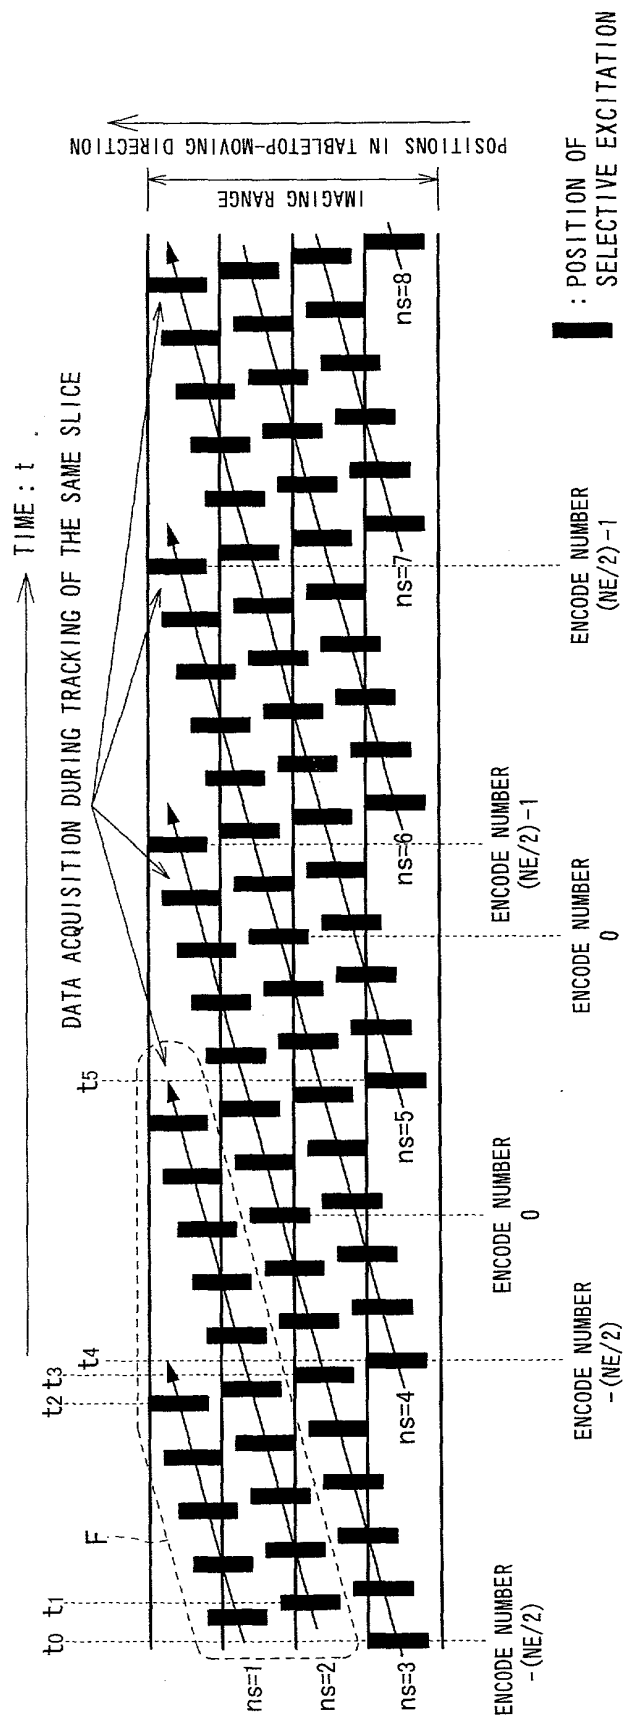

MULTI-SLICE IMAGING WITH TABLETOP MOVED
(NUMBER OF MULTI-SLICES = 3)

FIG. 2

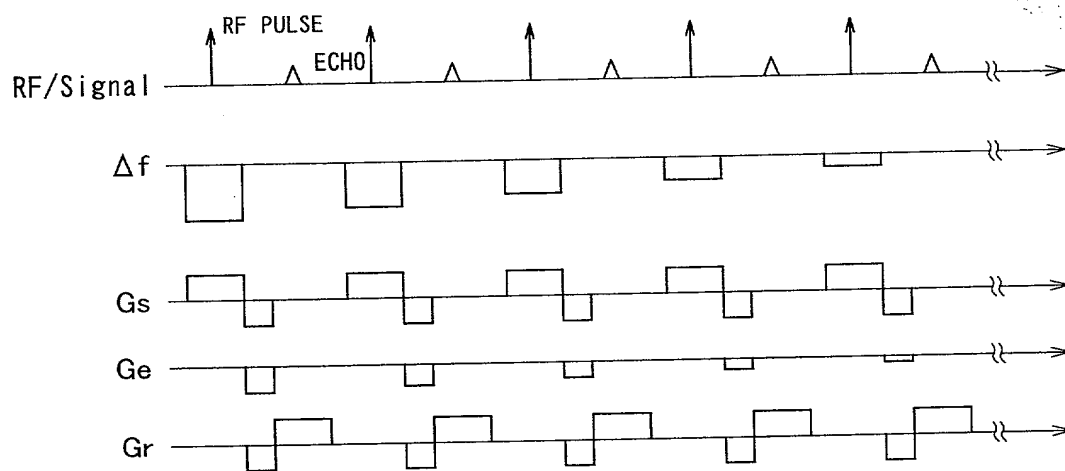


FIG. 3

FIG. 4A

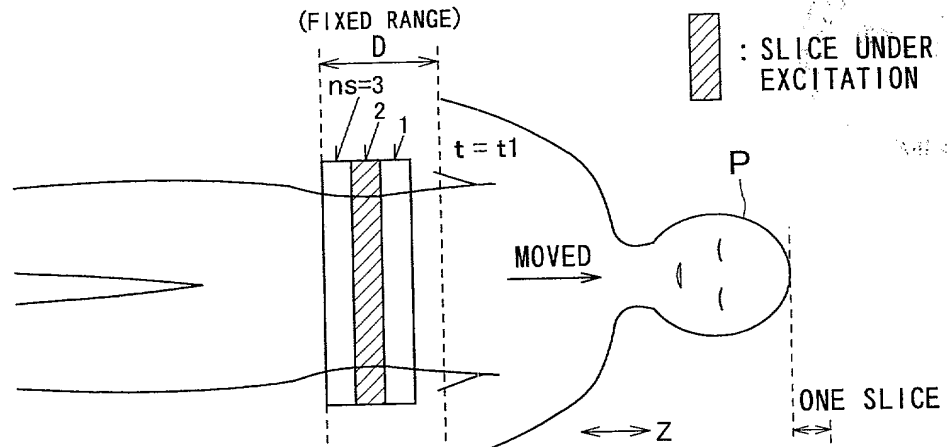


FIG. 4B

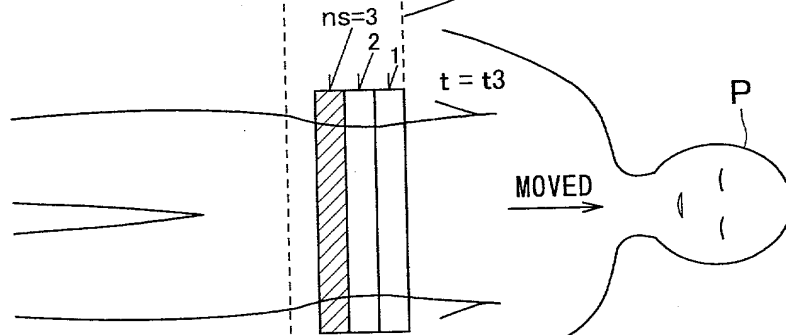


FIG. 4C

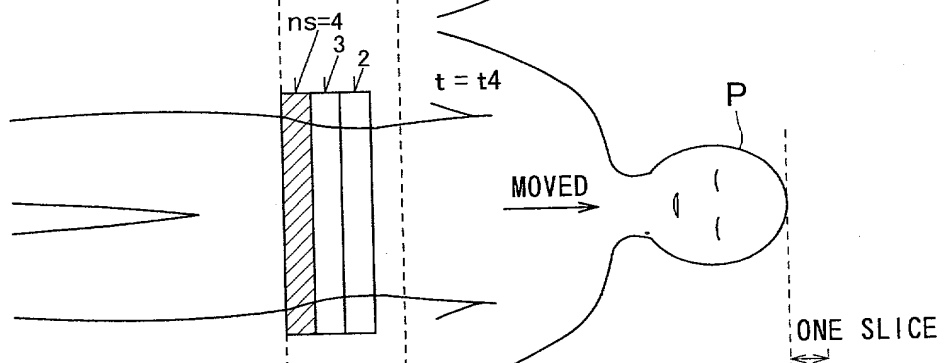
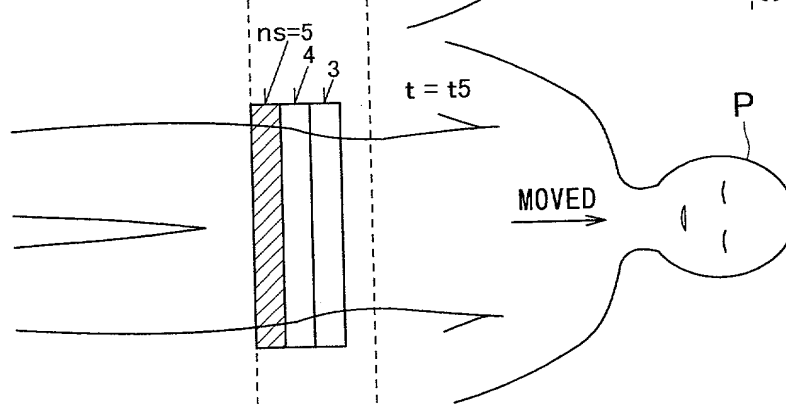


FIG. 4D



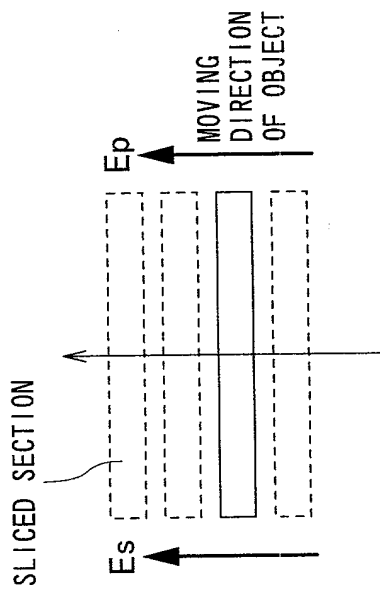


FIG. 5A

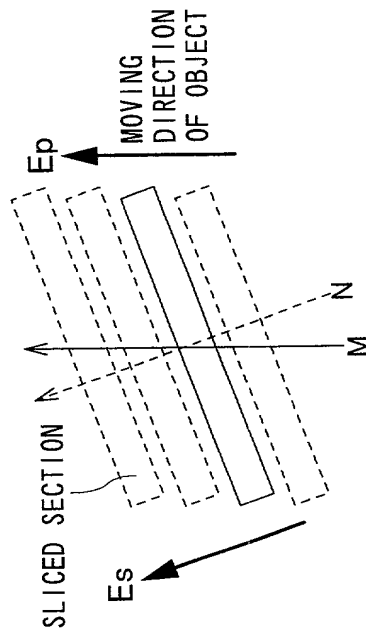


FIG. 5B

205040-1542560

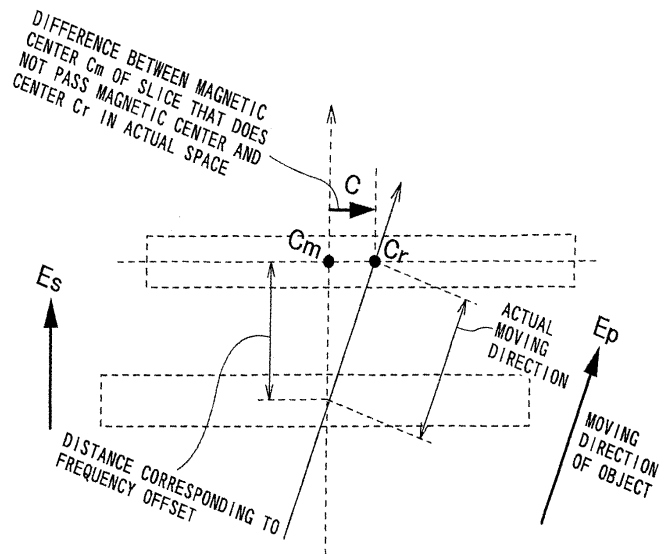


FIG. 6

FIG. 7A


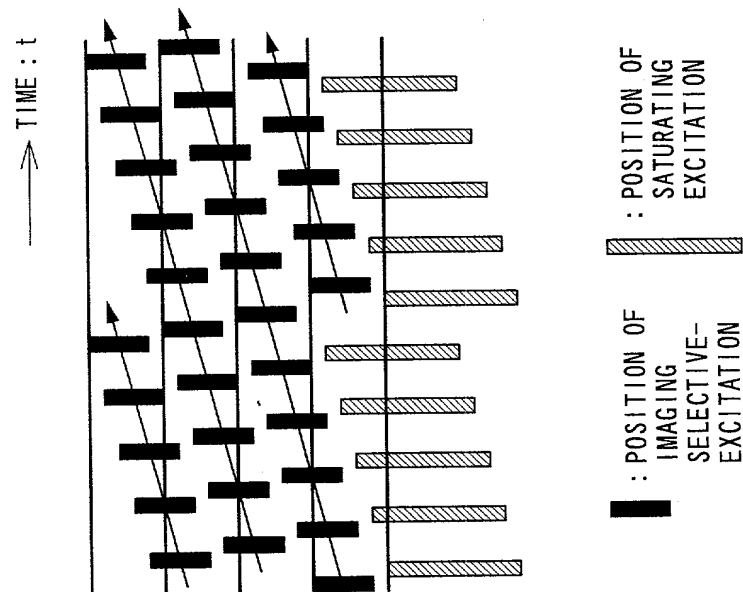


FIG. 7B

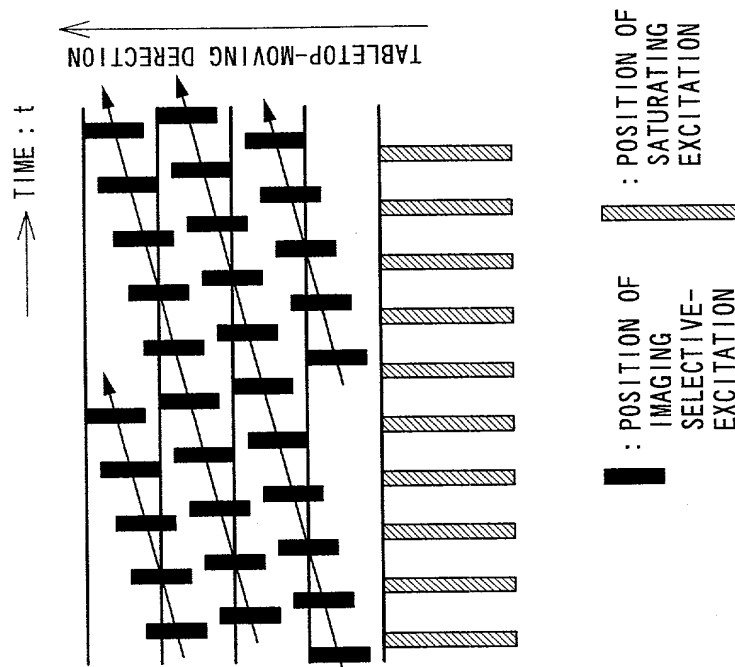

MULTI-SLICE IMAGING WITH TABLETOP MOVED
(USING PRE-SATURATION PULSE)